


MS Spectrum

Positive

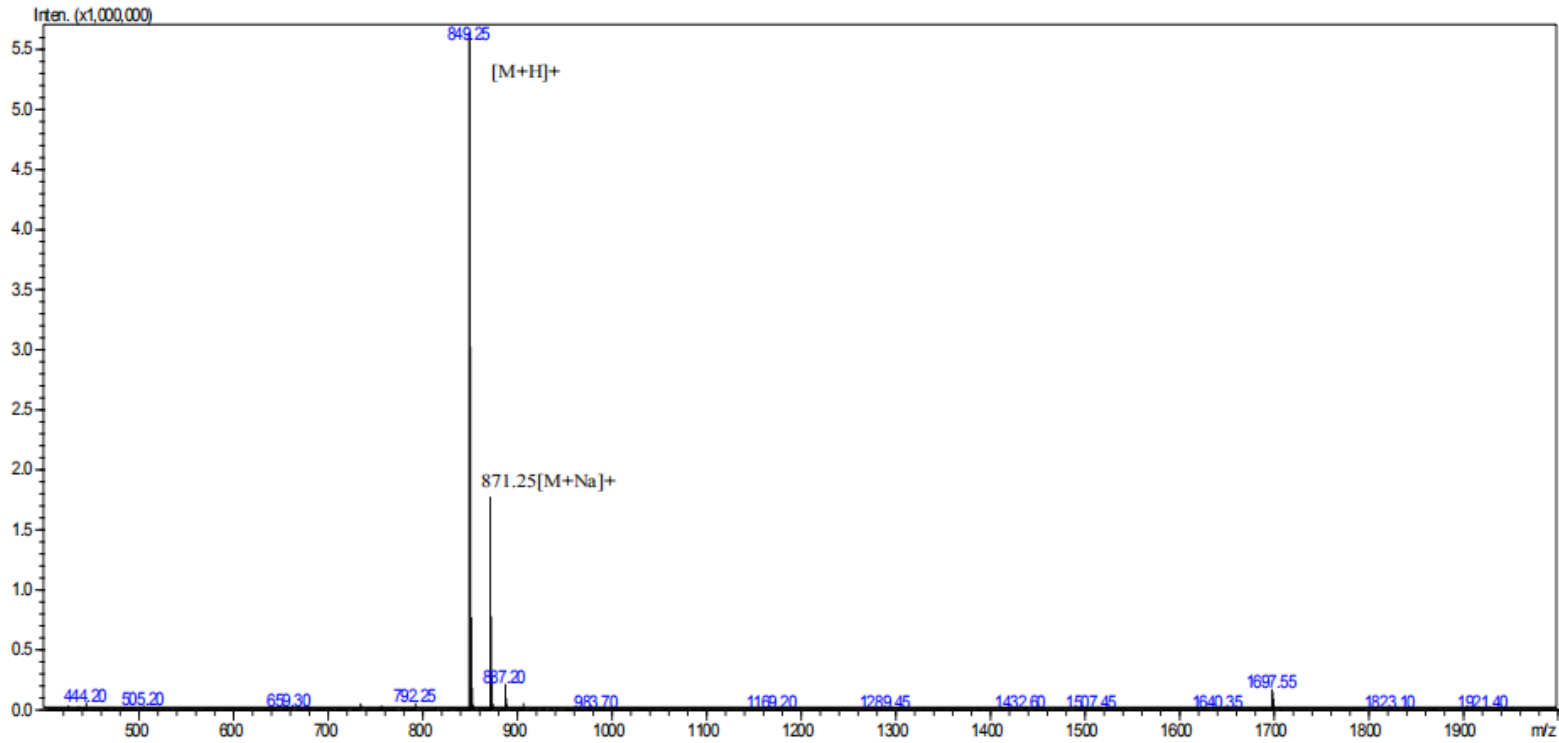

Sample Information

Date and Time

User

Sample

Inj. Volume

MW

Lot No.

: 2021-02-16 13:19:37

: SHAO

: 055319

: 1

: 848.81

: P170112-114-CQ055319

Probe:

Nebulizer Gas Flow:

CDL:

CDL Temp:

Block Temp:

ESI

1.5L/min

-20.0v

250°C

200°C

Probe bias:

Detector:

T. Flow:

B. conc:

-3.5kv

1.0kv

0.2ml/min

50%H2O/50%ACN