


MS Spectrum

Positive

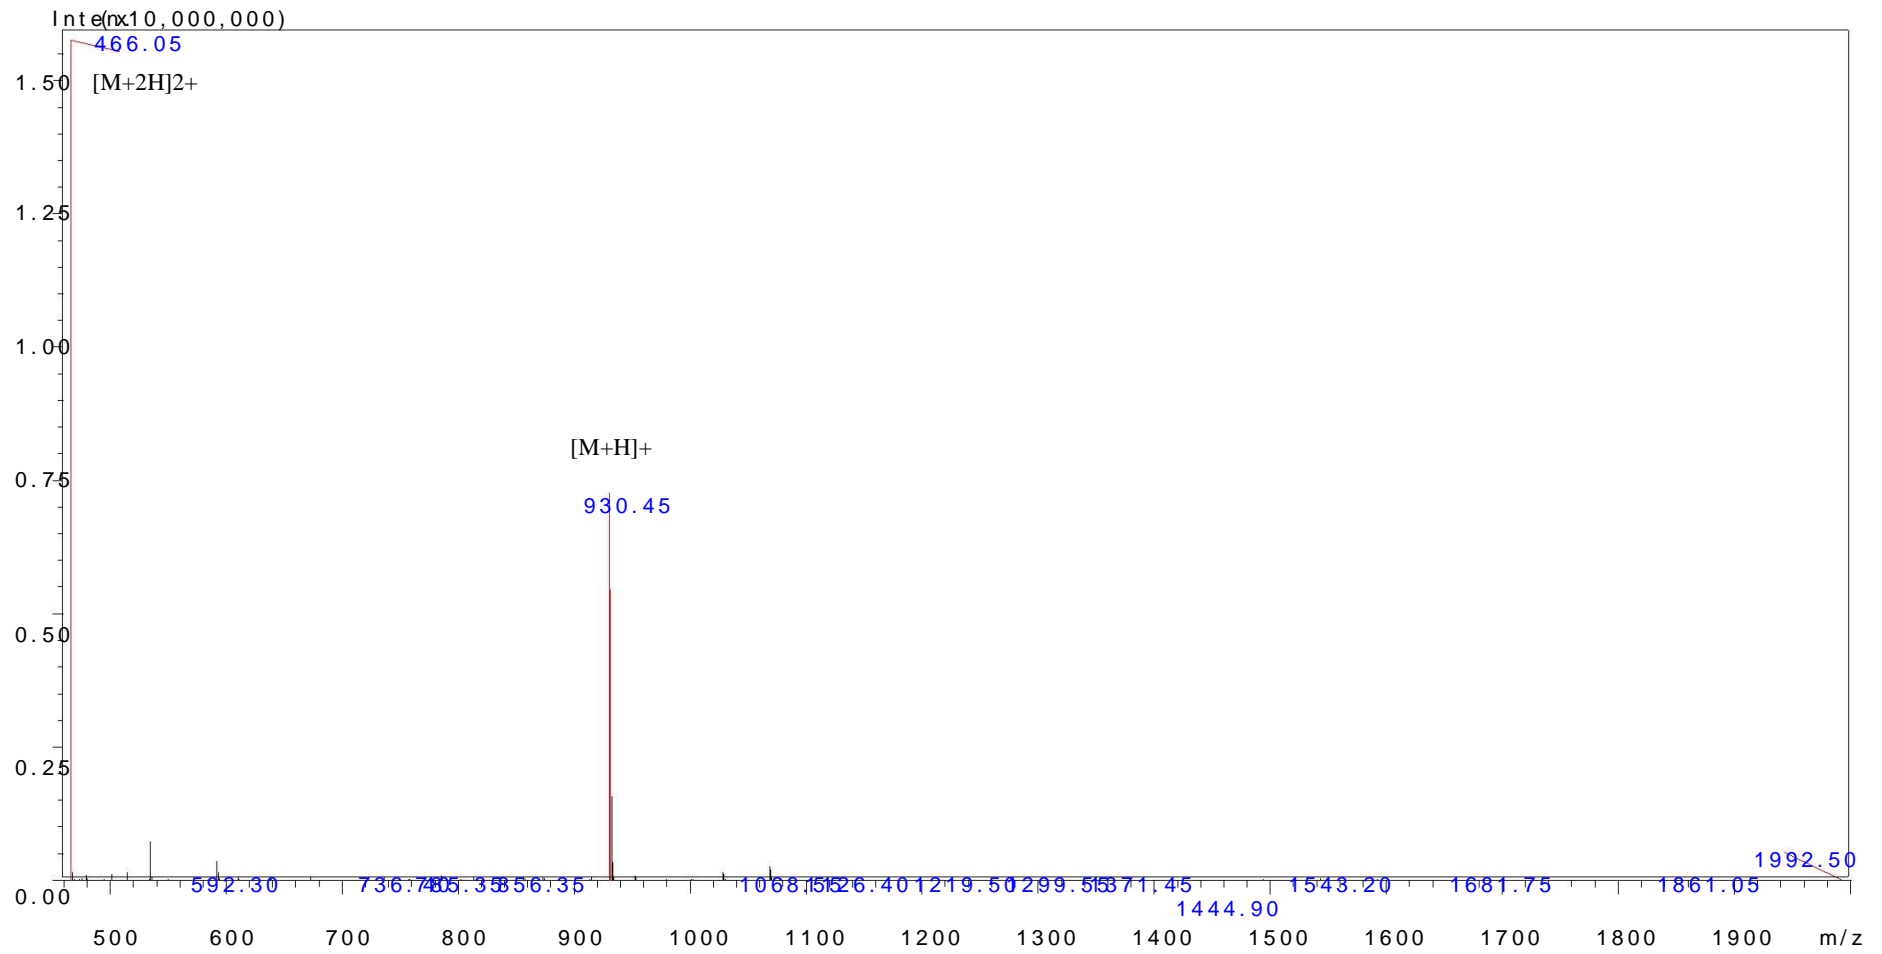

Data and Time : 2019/3/24
Sample : Peptide 2 GK-7-NH2
Inj. Volume : 1.000
Mw : 930.06
Lot No. : P190313-YS714329

Probe : ESI Probe bias : -4.5kv
Nebulizer Gas Flow : 1.5L/min Detector : 1.2kv
CDL : -20.0v T.Flow : 0.2ml/min
CDL Temp : 250°C B.conc : 50%H2O/50%ACN
Block Temp : 400°C