


Mass Spectrometry Report

4.70e6

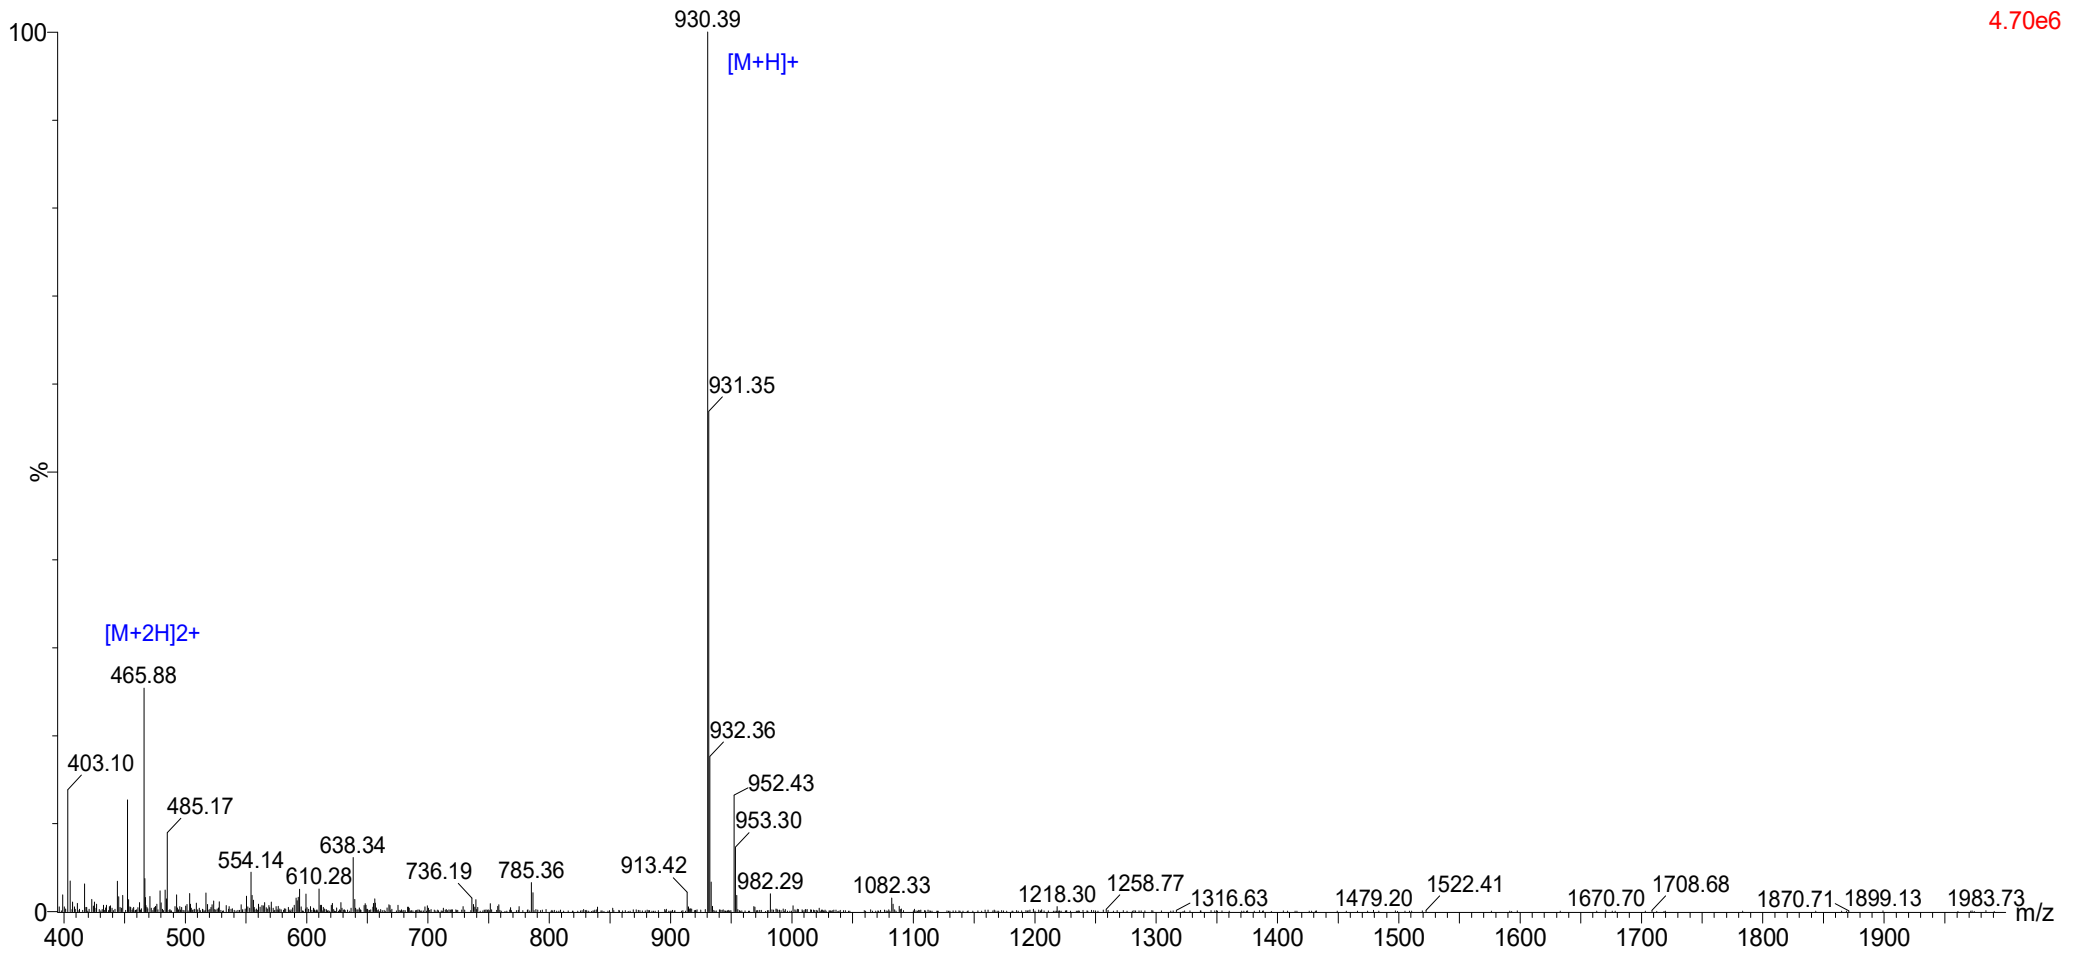

Sample Description

Analyzed date: 2020-12-14
Analyst: YU
Sample: 488708
M.W.: 930
Lot. No.: P200729-CQ488708

Instrument

Waters ZQ2000
Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
CDL Temp.: 250 °C
Block Temp.: 200 °C

Probe Bias: +4.5kv
Detector: 1.5kv
T. Flow: 0.2ml/min
B. Conc.: 50%H2O/50%ACN