


# MS Spectrum

Positive

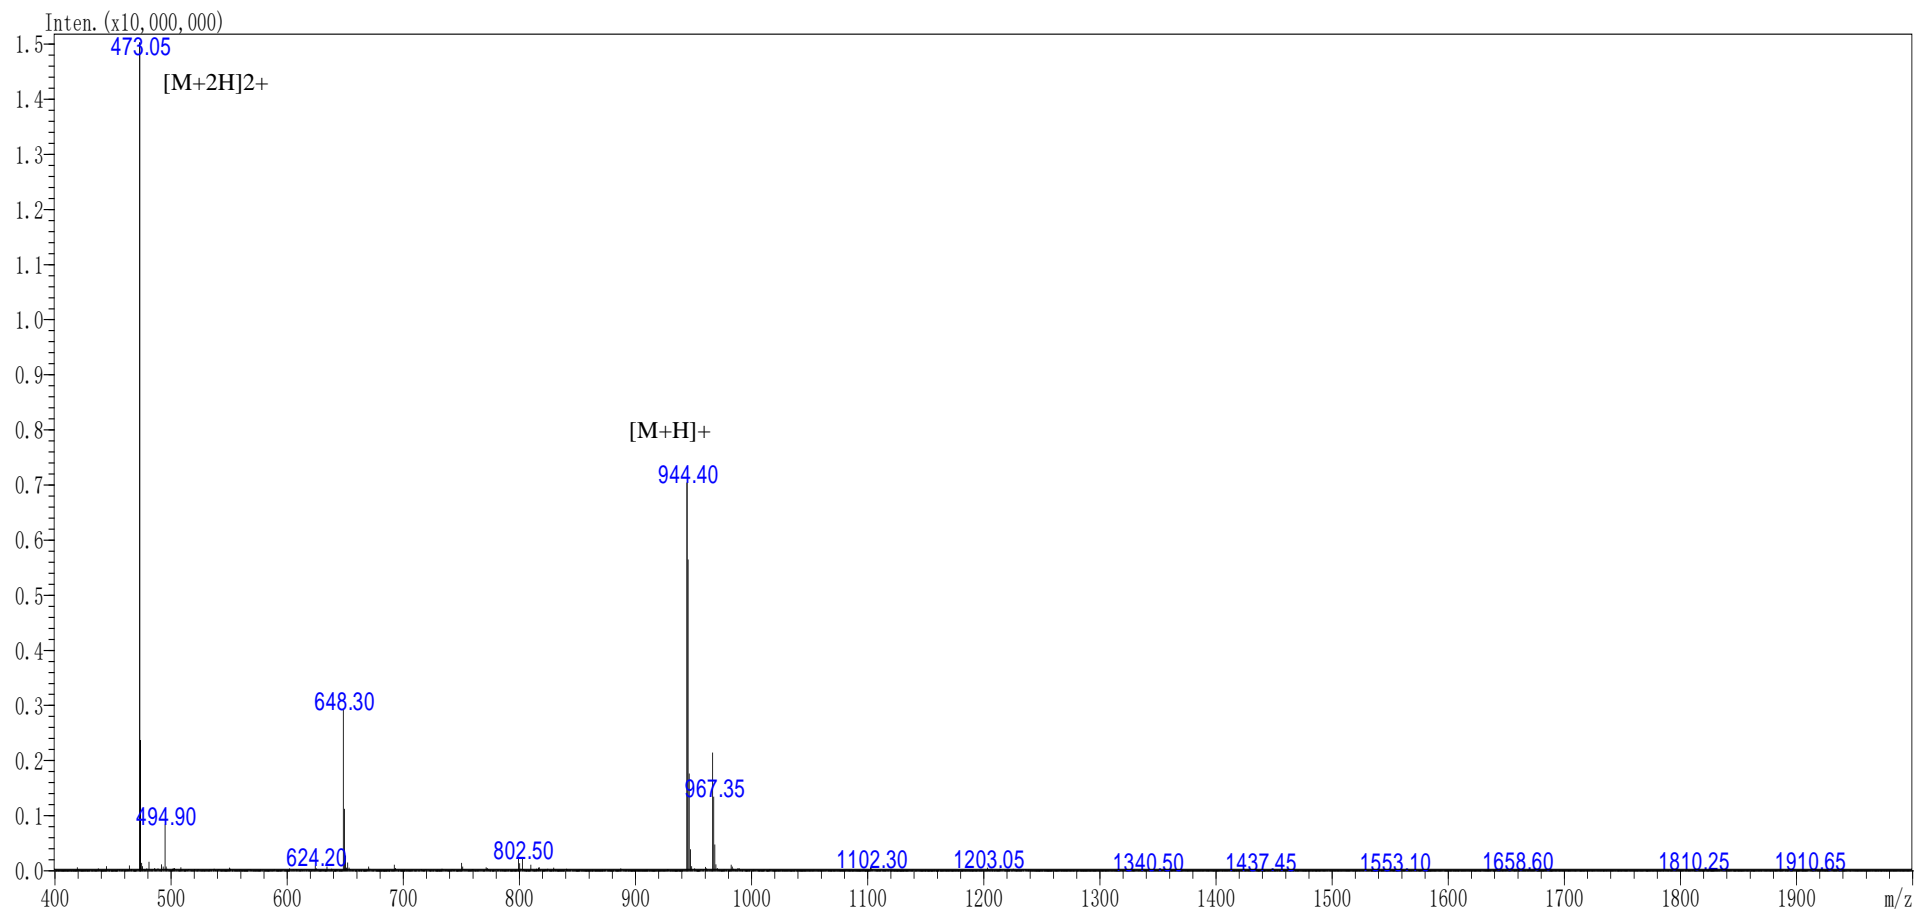

Acquired by :Shen  
Data Acquired : 2021/7/23  
Injection Volume : 1  
Sample Name : Peptide3 GK-7-NH2  
Mw : 944.11  
Lot No. : P210707-CQ714330

Probe :ESI  
Nebulizer Gas Flow :1.5L/min  
CDL :-20.0v  
CDL Temp :250°C  
Block Temp :400°C  
Probe bias :+4.5kv  
Detector :1.2kv  
T.Flow :0.2ml/min  
B.conc :50%H2O/50%ACN