


Mass Spectrum

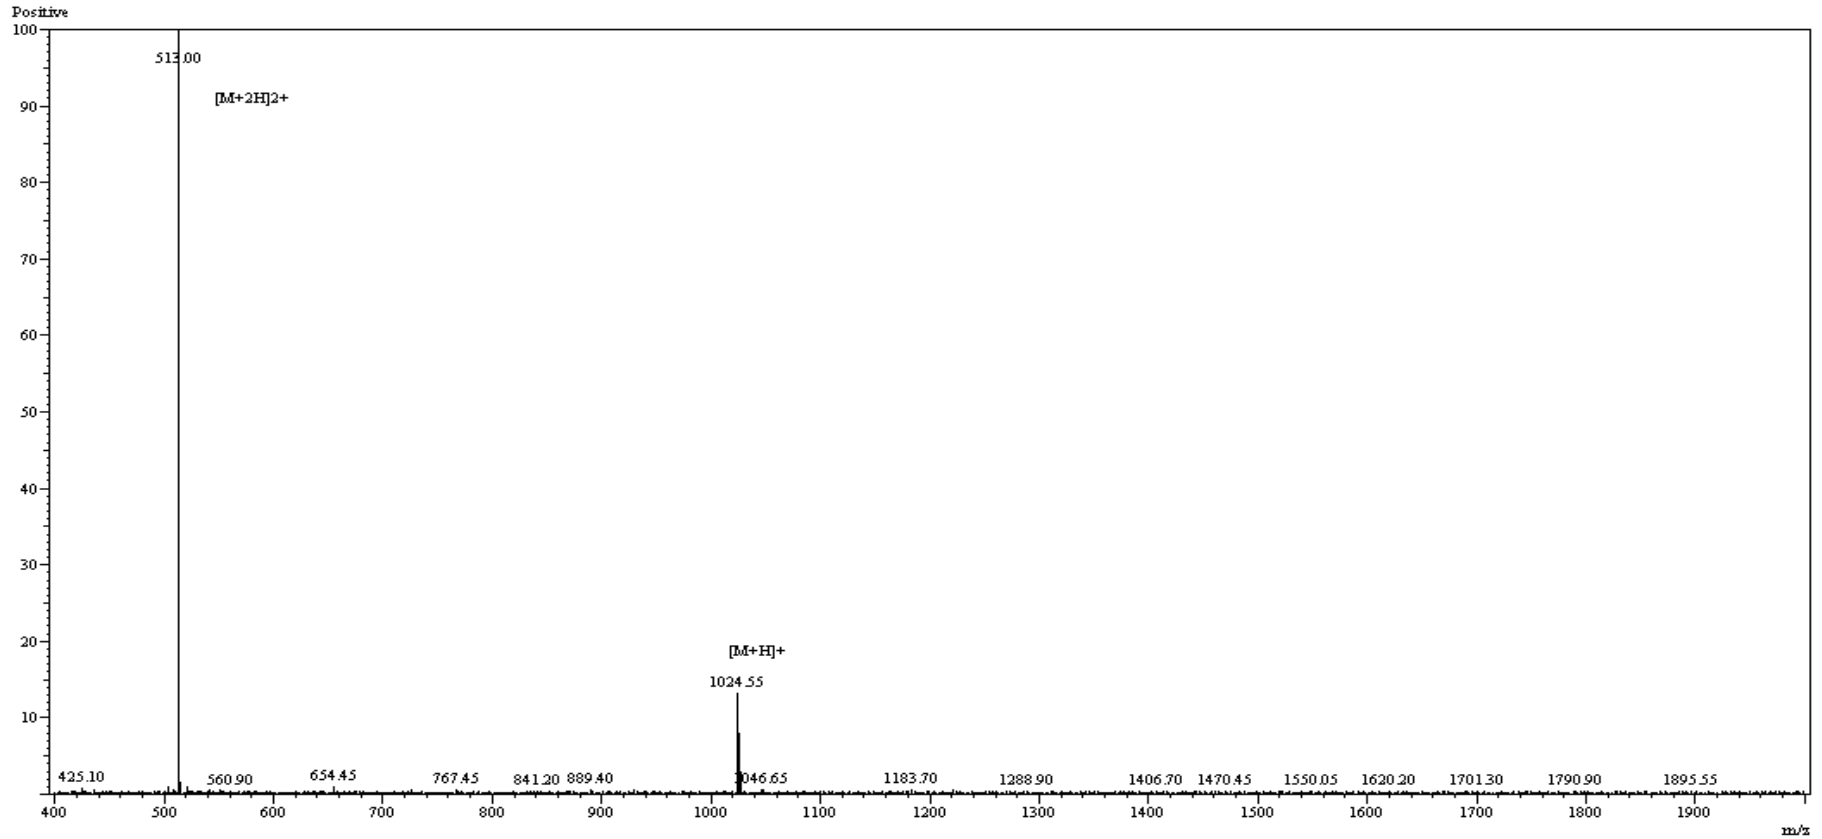

Sample Information

Date and Time : 2021-6-22 13:03:45
User : SHAO
Sample : MT2
Inj. Volume : 1
MW : 1024.2
Lot No. : P210512-MX477171

Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
CDL Temp: 250°C
Block Temp: 200°C

Probe bias: 3.5kv
Detector: 1.0kv
T. Flow: 0.2ml/min
B. conc: 50%H₂O/50%ACN