


MS Spectrum

Negative

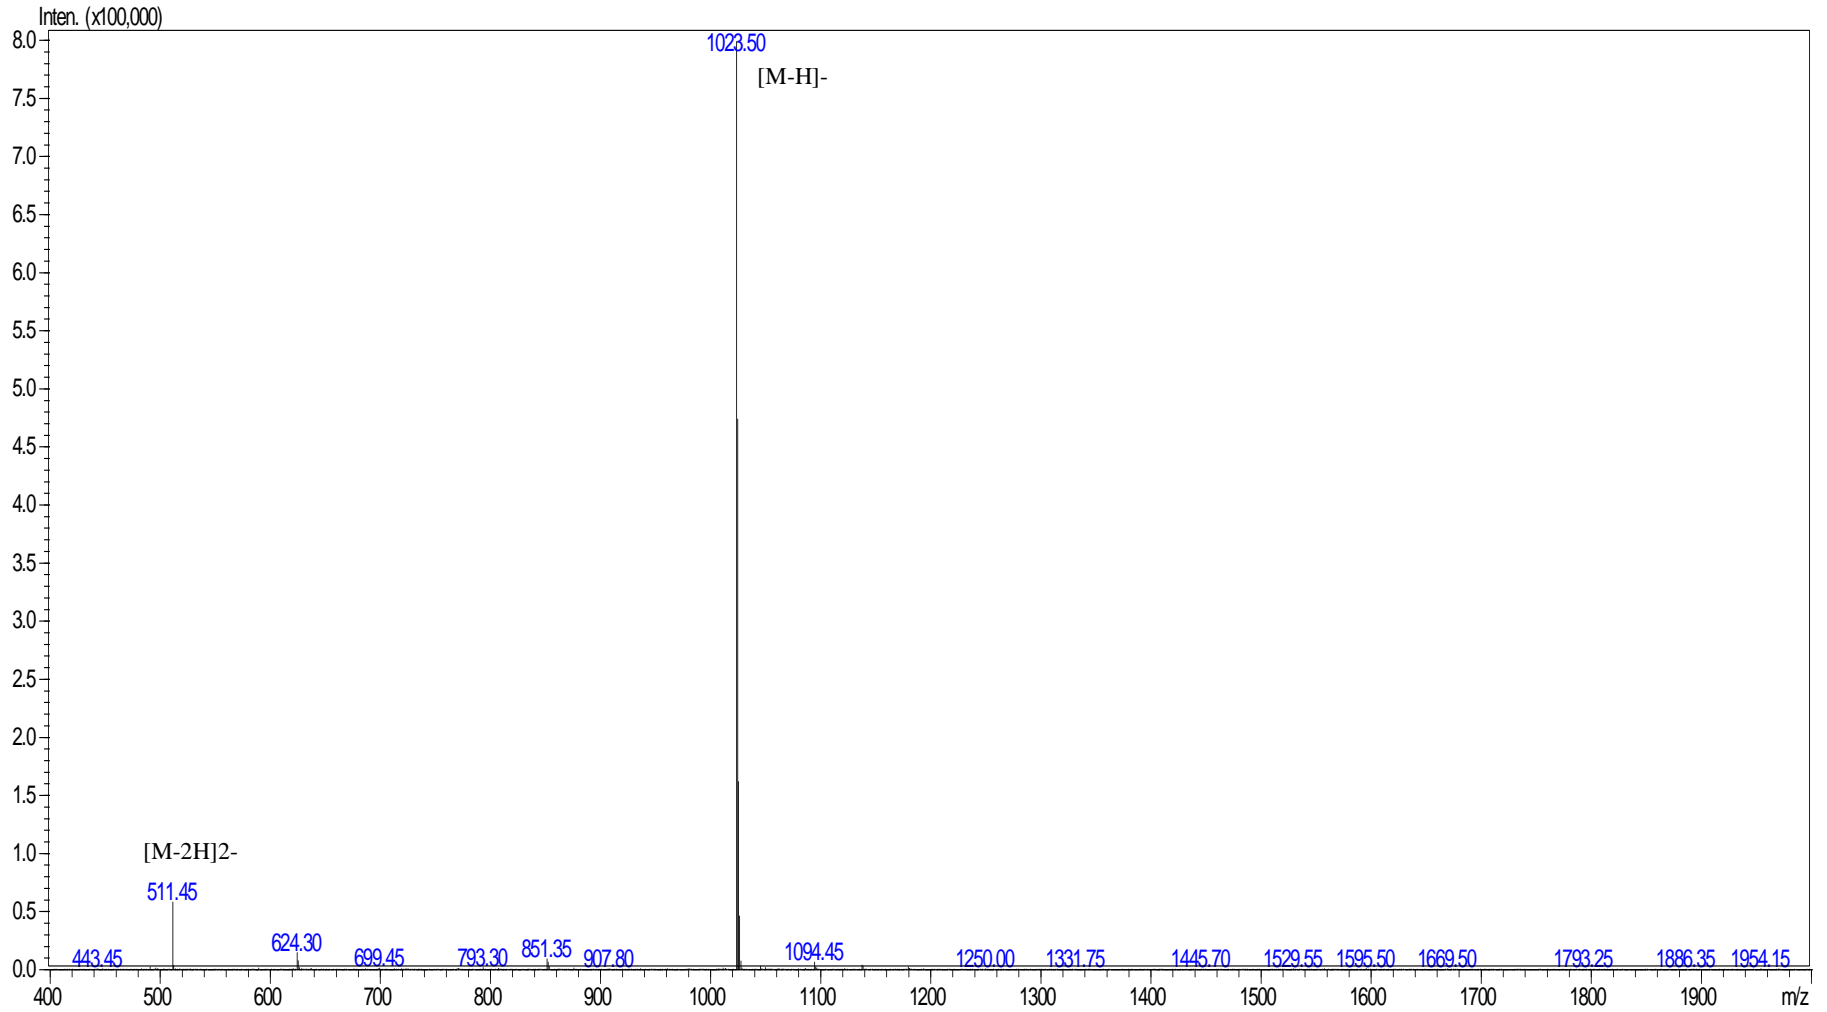

Acquired by :Shen
Data Acquired : 2021/7/27
Injection Volume : 1
Sample Name :
Mw : 1025.20
Lot No. : P210707-CQ471226

Probe :ESI
Nebulizer Gas Floe :1.5L/min
CDL :-20.0v
CDL Temp :250°C
Block Temp :400°C
Probe bias :+4.5kv
Detector :1.2kv
T.Flow :0.2ml/min
B.conc :50%H2O/50%ACN