


Mass Spectrometry Report

3.19e7

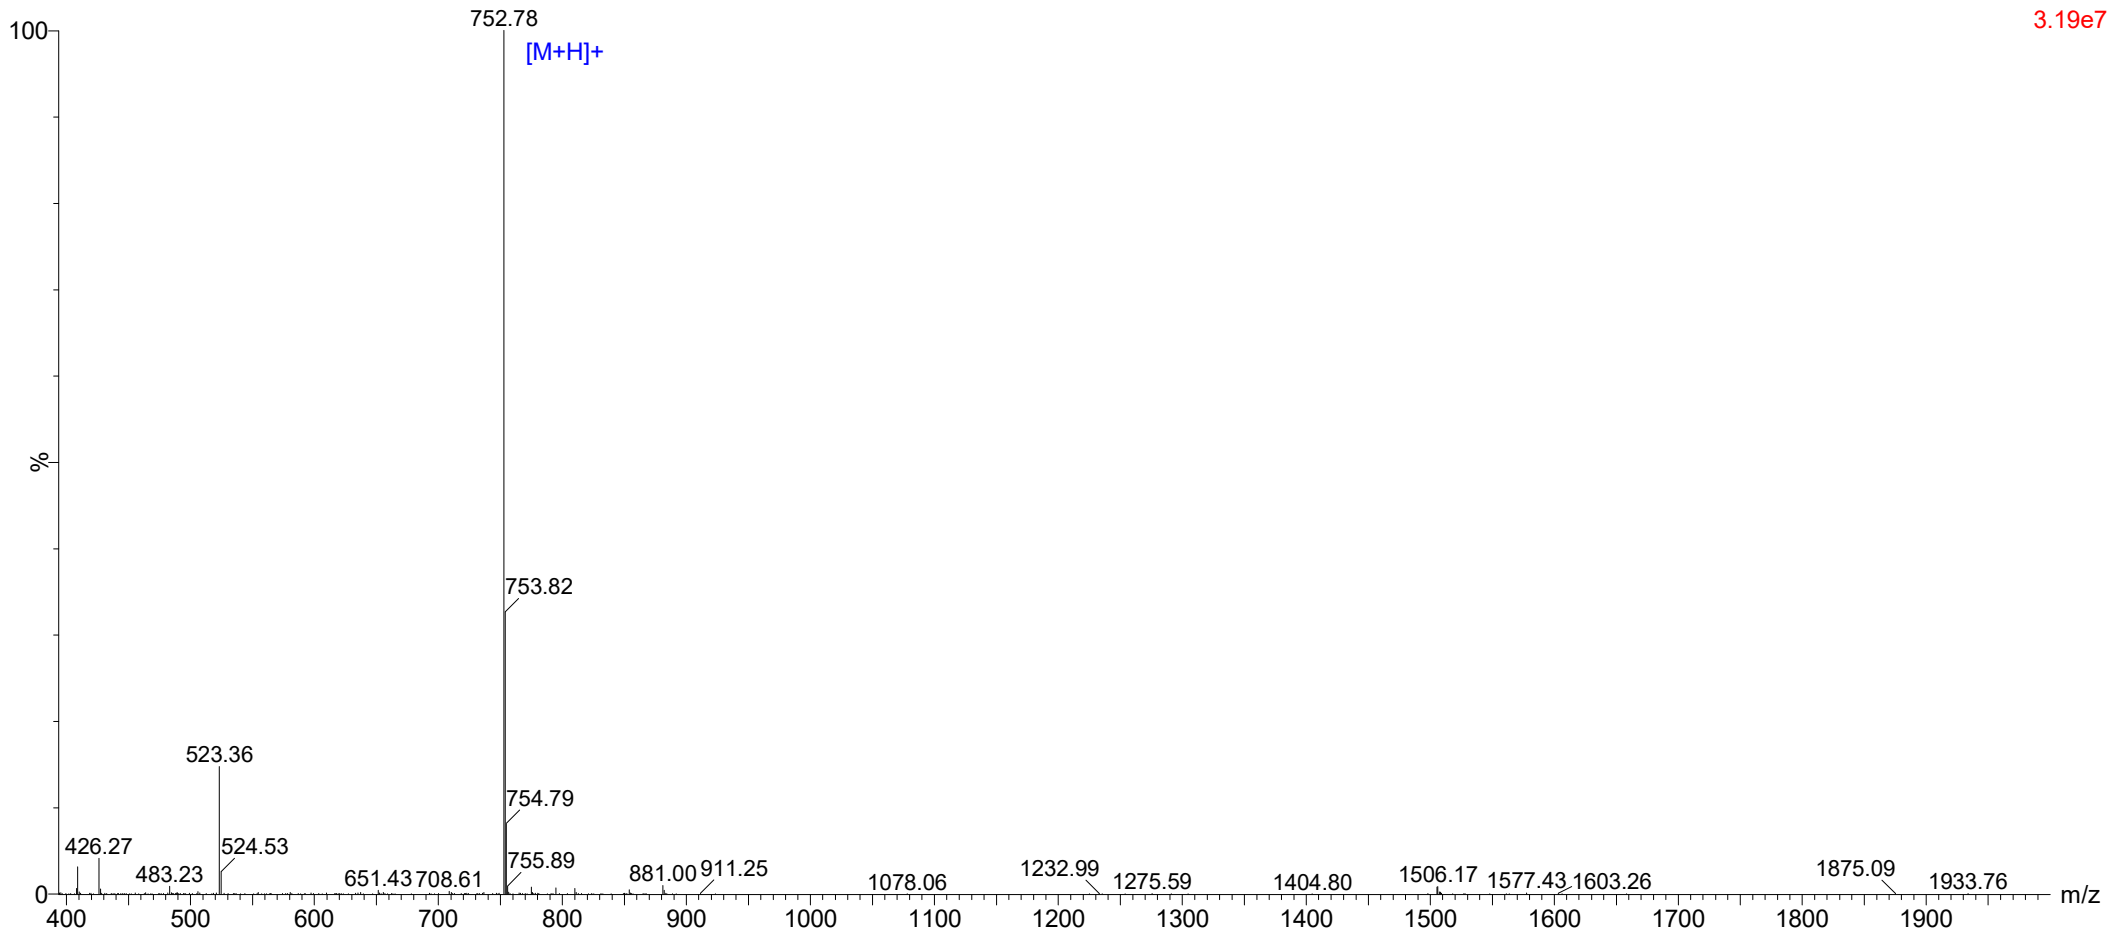

Sample Description

Analyzed date: 2020-5-10
Analyst: YU
Sample: 271657
M.W.: 751.89
Lot. No.: P140605-88-CQ271657

Instrument

Waters ZQ2000
Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
CDL Temp.: 250 °C
Block Temp.: 200 °C

Probe Bias: +4.5kv
Detector: 1.5kv
T. Flow: 0.2ml/min
B. Conc.: 50%H2O/50%ACN