Injection Data File Directory /2022/2021062803/Results/220524/002.rslt

Sample Description Sample ID:817031 Lot#:CV-05-00100
Mobie Phase:A:0.1%TFA in H2O
B:0.09%TFA in (80%ACN+20%H20)
Flow:1.0ml/min 26.0%-36.0% B buffer in 20min
Column:SepaxGP-C18 5u 120A 4.6*150mm A2181#

Injection Acquired Date	5/24/2022	Sample Vial Number	P1-A4
Injection Acquired By	amy shi	Injection Volume	2.000
Instrument Name	2021062803	Injection Volume Unit	µL

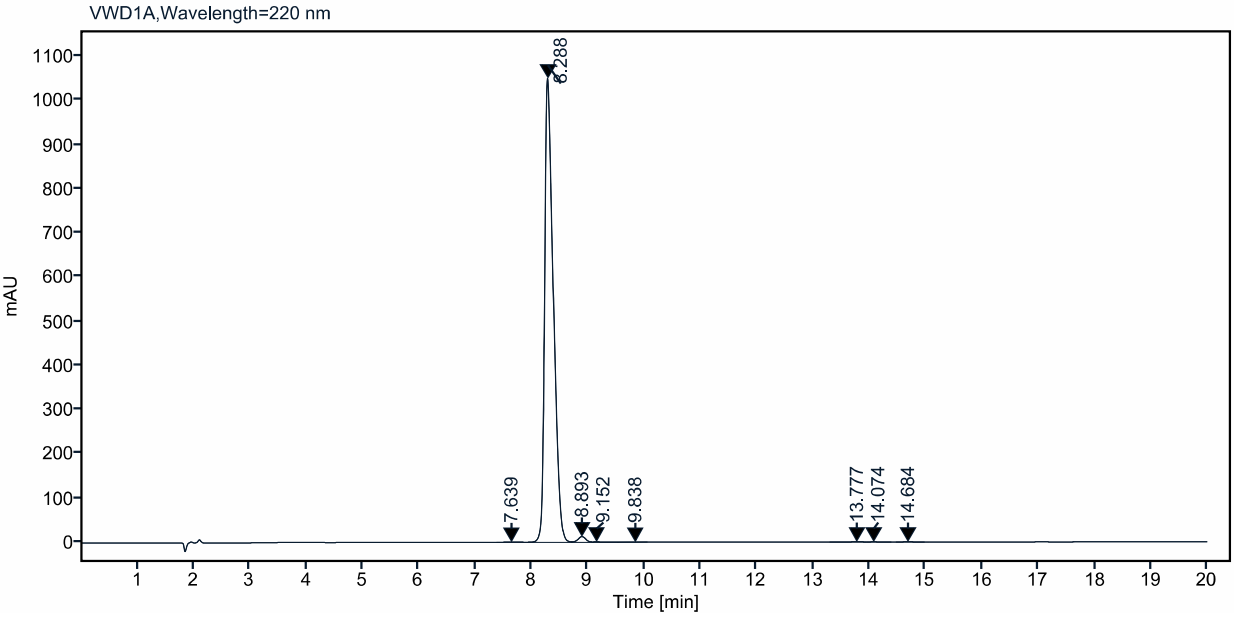

Signal: VWD1A,Wavelength=220 nm

RT [min]	Type	Width [min]	Height	Area	Area%
7.639	BV	0.520	0.842	12.268	0.107
8.288	VV	0.818	1050.970	11310.023	98.480
8.893	VV	0.378	12.692	124.756	1.086
9.152	VV	0.442	1.010	9.500	0.083
9.838	VBA	0.518	0.360	3.651	0.032
13.777	BV	0.659	0.766	12.017	0.105
14.074	VBA	0.431	0.407	5.402	0.047
14.684	BBA	0.507	0.674	6.972	0.061