

# ANALYTICAL CERTIFICATE

Page 1/8

<b>Sample name</b>	<b>PT-141</b>
<b>Batch No.</b>	<b>2025233</b>
<b>Sample No.</b>	<b>01</b>
<b>Sequence</b>	Ac-Nle-cyclo[Asp-His-D-Phe-Arg-Trp-Lys]-OH
<b>Manufacturing date</b>	<b>NA</b>
<b>Submitter of analytical request</b>	<b>Particle s.r.o., Slovakia</b>

## 1. Peptide content by HPLC/CLND:

### 1.1 HPLC Instrument:

Pump: Agilent 1200 Series, Quat Pump G1311A  
Sampler: Agilent 1260 Series, Hip ALS G1367E  
Degasser: Agilent 1200 Series, Degasser G1379B  
Detectors: Agilent 1200 Series, VWD G1314B  
Nitrogen detector Antek 8060

### 1.2 HPLC conditions:

Eluents: A – MilliQ water  
B – isopropanol  
D – 1% TFA in MilliQ water  
Flow rate: 1 mL/min  
Gradient:

Time	A (%)	B (%)	D (%)
0	90	0	10
1	90	0	10
9	10	80	10
10	10	80	10
11	90	0	10
15	90	0	10

Column: ARION 5 $\mu$  C4-BIO 300 A, 4.6 x 100 mm  
Serial No 221258

### 1.3 Sample preparation:

The whole amount of PT-141 (10 mg) was dissolved in 2 mL of DMSO.  
Injection: 2.0  $\mu$ L


# ANALYTICAL CERTIFICATE

Page 2/8

## 1.4 Chromatograms and calibration curve:

Instrument: CLND-2 Sequence: 250320

Page 1 of 2

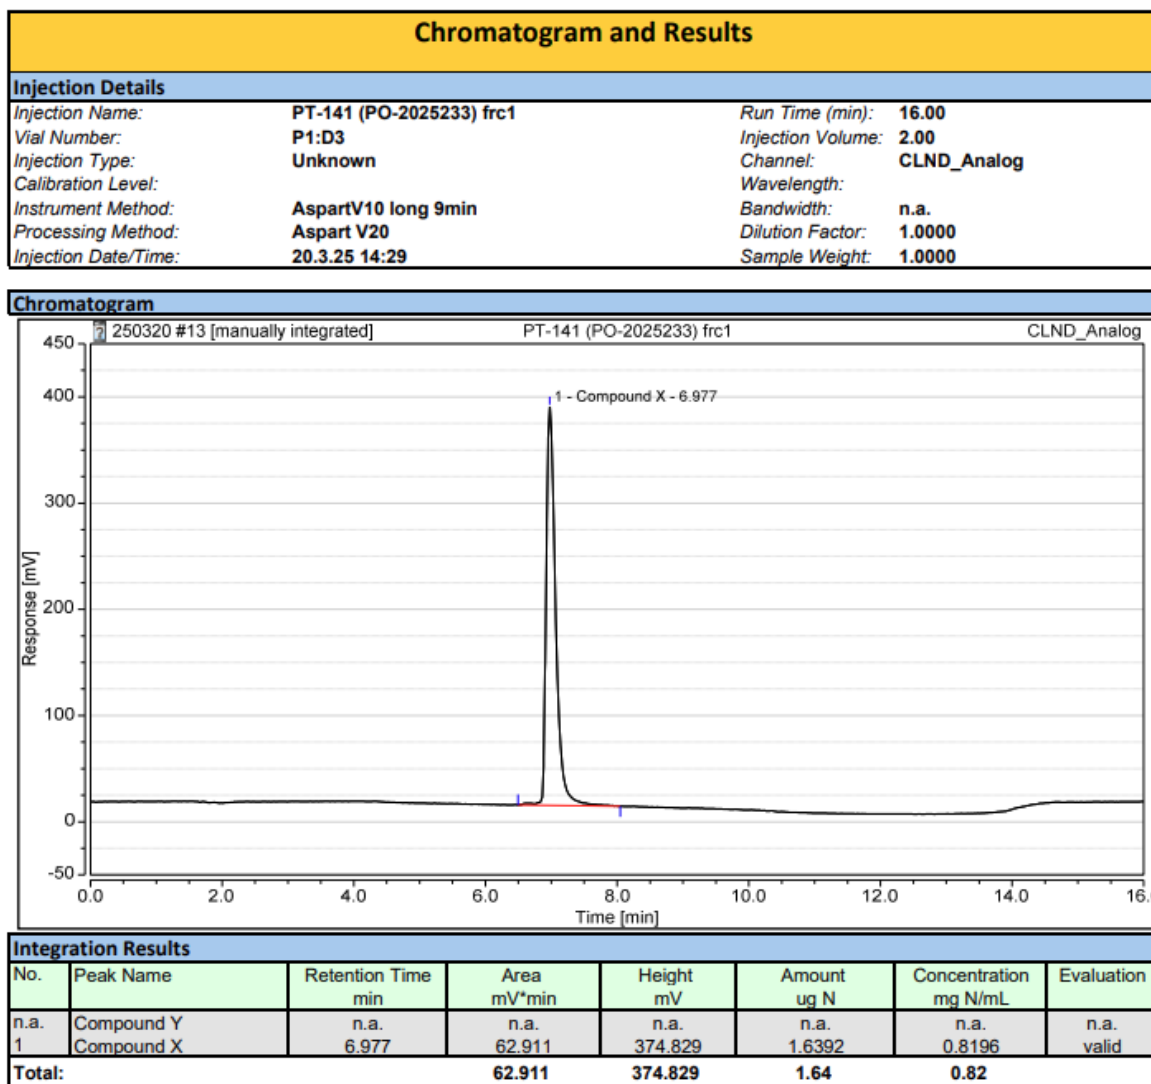


# ANALYTICAL CERTIFICATE

Page 3/8

Instrument: CLND-2 Sequence: 250320

Page 1 of 2

Chromatogram and Results			
Injection Details			
Injection Name:	PT-141 (PO-2025233) frc2	Run Time (min):	16.00
Vial Number:	P1:D3	Injection Volume:	2.00
Injection Type:	Unknown	Channel:	CLND_Analog
Calibration Level:		Wavelength:	
Instrument Method:	AspartV10 long 9min	Bandwidth:	n.a.
Processing Method:	Aspart V20	Dilution Factor:	1.0000
Injection Date/Time:	20.3.25 15:24	Sample Weight:	1.0000

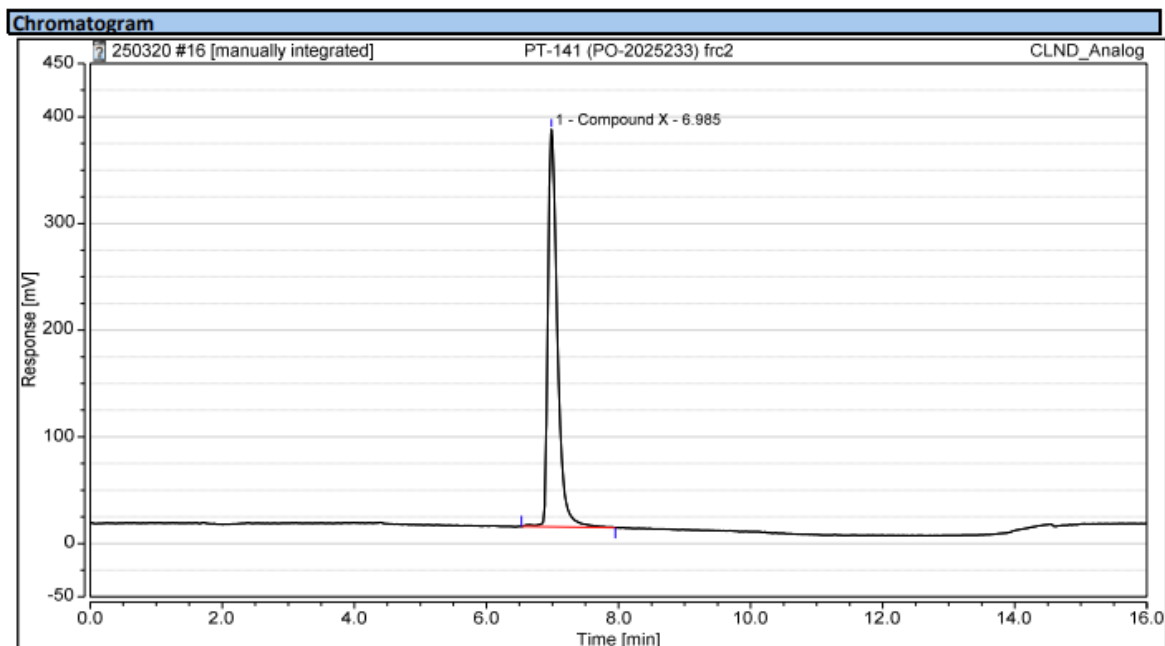


Integration Results							
No.	Peak Name	Retention Time min	Area mV*min	Height mV	Amount ug N	Concentration mg N/mL	Evaluation
n.a.	Compound Y	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
1	Compound X	6.985	62.422	372.272	1.6270	0.8135	valid
<b>Total:</b>			<b>62.422</b>	<b>372.272</b>	<b>1.63</b>	<b>0.81</b>	

# ANALYTICAL CERTIFICATE

Page 4/8

Instrument: CLND-2 Sequence: 250320

Page 2 of 2

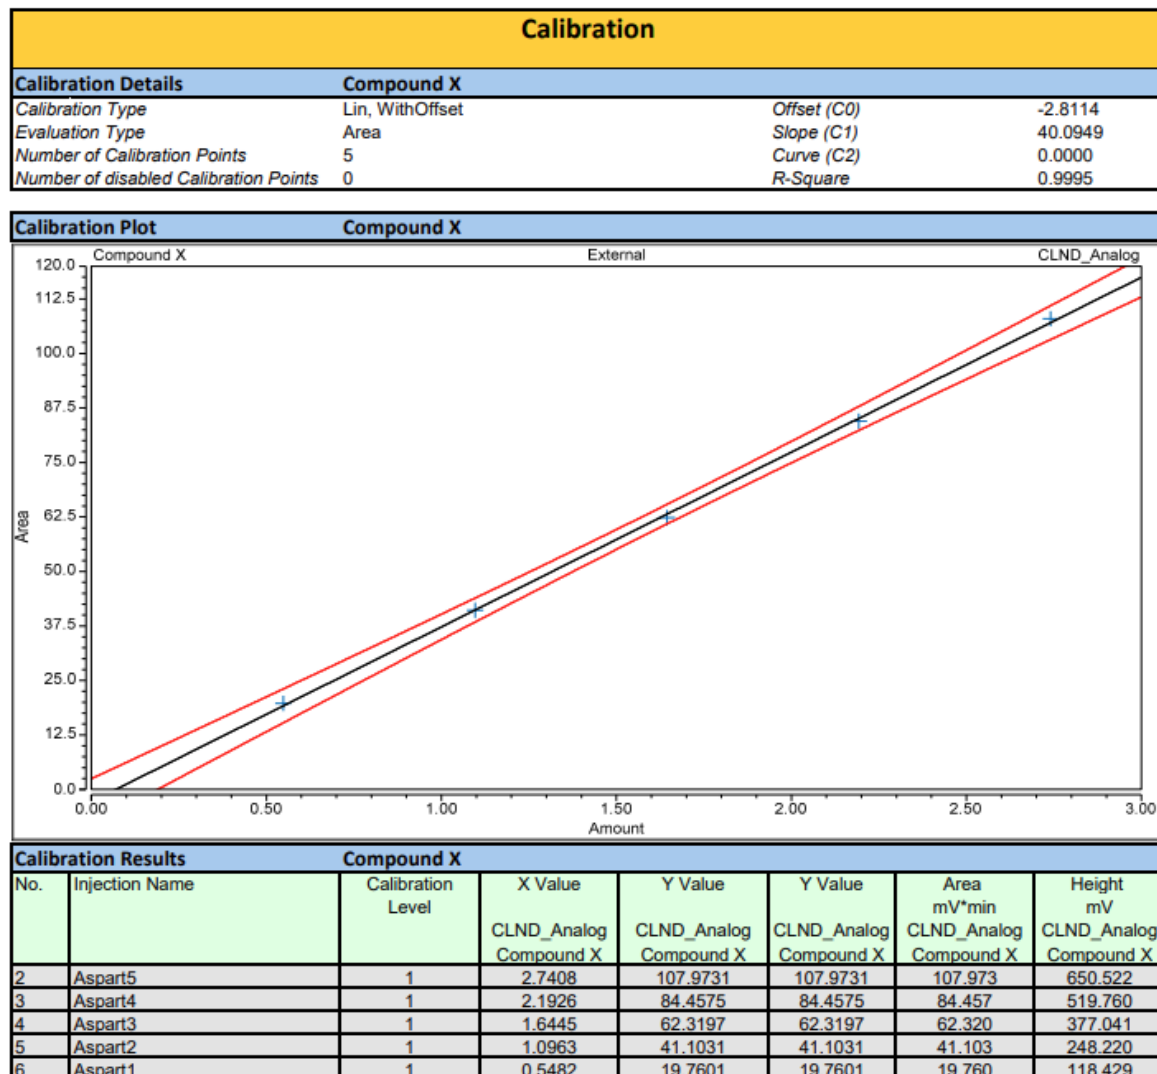

## ANALYTICAL CERTIFICATE

Page 5/8

### 1.4 Results:

NNC: PT-141 (PO-2025233)		Salt:	0
MW <i>(calculated)</i> g/mol	N content <i>(calculated)</i> %	N conc. <i>(measured)</i> mg × N/ml	
1025,18	19,13	0,8166	
Theoretical Volume ml		Lyophilizate amount mg	
2,00		10,00	
Peptide concentration mg/ml		Quantified amount mg	
4,27	4164	8,5	8 327
Peptide content assay %			
85,4			

### Summary table:

Peptide	Aliquoting (mg)	Total weight of sample (mg)	Content of the peptide by CLND (mg)	Content of the peptide in the sample (%)	Content of the peptide against the amount on label.
PT-141	10	NA	<b>8,5</b>	NA	85,4 %

## **ANALYTICAL CERTIFICATE**

Page 6/8

### **2. Purity assessment by UPLC:**

#### **2.1 HPLC Instrument:**

LC-System                Waters Acquity UPLC  
Detectors:              UV or DAD at 214 nm

#### **2.2 HPLC conditions:**

Eluents:                A – MilliQ water + 0.05% TFA  
                              B – acetonitrile + 0.05% TFA  
Flow rate:             0.45 mL/min  
Gradient:              from 5% B to 60% B in 4 min, according to chromatogram results  
Column:                Waters Acquity BEH, C-18, 1.7µm, 2.1mm x 50mm

#### **2.3 Sample preparation:**

An aliquote of PT-141 (1 mg) was dissolved in 1 mL of water.  
Injection:              0.3 µL

# ANALYTICAL CERTIFICATE

Page 7/8

## 2.4 Chromatogram of PT-141 (PO2025233)

### Sample information

#### UPLC5

Channel Description PDA Ch1 214nm@4.8nm

Vial : 1:C,3 Vol. : 0.30 ul


**Sample: PT-141 (PO-2025233)**

Date Acquired 3/18/2025 4:26:20 PM CET

Date Processed 3/19/2025 2:17:02 PM CET

Acq Method Set :

Gr5\_60\_4mi\_40C\_0\_45ml\_K2\_met\_s

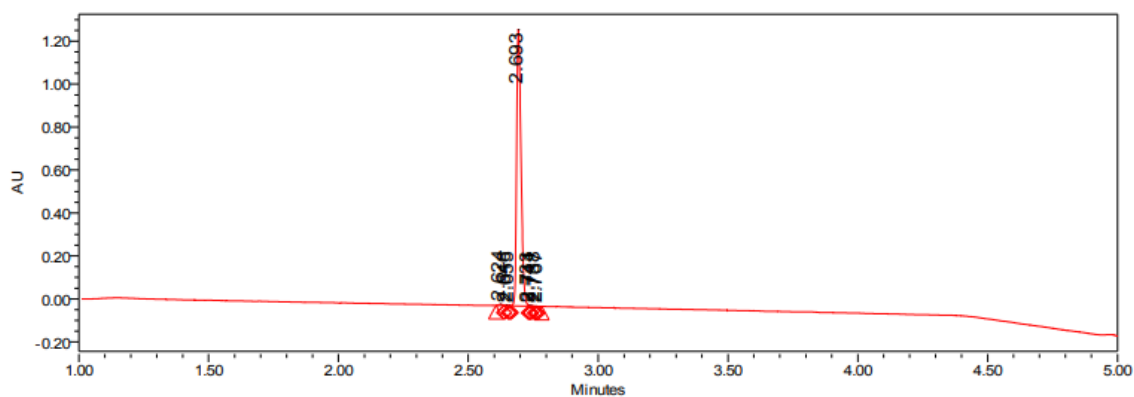

	RT	Area	Height (μV)	% Area
1	2.624	6611	6923	0.43
2	2.693	1514170	1286528	99.13

A: 0.05% TFA in water

B: 0.05% TFA in acetonitrile

Gradient :

0.0 - 0.5min 5 - 5 % B

0.5 - 4 min 5 - 60 % B

4.0 - 4.5 min 60 - 100 % B

4.5 - 5.0min 100 % B

5.0 - 5.5min 100 - 5 % B

6min 5 % B

0.45ml/min

Acquity UPLC BEHC18, 1.7μm, 2.1 x 50 mm column

column oven temp. = 40 °C

## 2.5 Result of purity assessment

The overall purity is 99.13 % at 214 nm.

## ANALYTICAL CERTIFICATE

Page 8/8

### 3. Endotoxin test:

#### 3.1 Description:

Test tubes: Gel Clot Lyophilized Amebocyte Lysate Single Test in Vial  
Manufacturer: Xiamen Bioendo Technology Co., Ltd.  
Lot: 24061152  
Content: 0.2 ml endotoxin-specific Amebocyte Lysate which includes beta-glucan inhibitor in the formulation  
Sensitivity of test: 0.5 EU/mL  
Sample sensitivity level: 5 EU/mg

#### 3.2 Sample preparation and test:

A sample peptide is dissolved in endotoxin-free water to form a concentration of 0.5 mg/mL. 200 µL of this solution is then transferred to the Amebocyte Lysate Single Test tube and incubated at 37 °C for 60 min. Immediately after incubation the test tube is slowly turned upside down.

A solid gel clot which doesn't come down immediately indicates **positive** result (meaning that endotoxins are above the current sensitivity level).

An absence of solid gel clot so the solution freely flows down from the bottom of test tube indicates **negative** result (meaning that endotoxin are below the current sensitivity level).

#### 3.3 Result:

NEGATIVE (-)


#### CONCLUSION:

**The sample PT-141 (Batch No. 2025233) was analyzed for peptide content, UV purity and endotoxins.**

**Peptide content is 85.4 % (8.5 mg in 10 mg)**

**Purity is 99.13 % (UPLC at 214 nm).**

**Endotoxin test (sensitivity level 5 EU/mg) - NEGATIVE.**
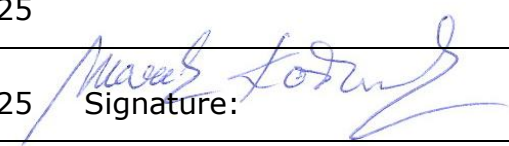
<b>ANALYSIS COMPLETED:</b>	Date: 19.03.2025
<b>Issued by QC:</b>	Date: 26.03.2025  Signature:

## Analytical report AR-25-KT-009256-03



## Testing laboratory:

Eurofins Environment Testing Slovakia s.r.o.  
 Robotnícka 820/36, 039 01 Turčianske Teplice  
 IČO: 53 248 376  
 Place of work:  
**Accredited testing laboratory Turčianske Teplice**  
 Robotnícka 820/36, 039 01 Turčianske Teplice  
 tel: 043/490 1562  
 RegistrationEnviroSK@etcee.eurofins.com, www.eurofins.sk

## Customer:

PARTICLE s.r.o.  
 Kolonáda 4490/18  
 984 01 Lučenec  
 SLOVAKIA

Date of Sample Receipt: 17.03.2025 Date of Testing: 17.03.2025 - 20.03.2025

Issue date: 27.03.2025

## Information about Sampling:

Sampler: customer

Sample information: 104-2025-00009985

# Sample description: PT-141 (PO-2025233)

Material: Peptidy

## Physical and chemical tests

Parameter	Unit	Allowed Value	Measured Value	Uncertainty of Method measurement*	Testing method	E	SL	TT
Arsenic (As)	mg/kg	-	<1,50	-	ICP-MS	LS-PP-CH-85	-	TR A
Cadmium (Cd)	mg/kg	-	<0,20	-	ICP-MS	LS-PP-CH-85	-	TR A
Lead (Pb)	mg/kg	-	<0,50	-	ICP-MS	LS-PP-CH-85	-	TR A
Mercury (Hg)	mg/kg	-	<0,30	-	ICP-MS	LS-PP-CH-85	-	TR A

## Notes:

E - evaluation  
 S - satisfied  
 NS - not satisfied  
 (A) - accredited sampling  
 (SA) - accredited sampling executed under the subcontract  
 ŠPP - Standard operation procedure  
 ND - not detected by given method  
 LOQ, LQ – limit of quantification  
 CFU - Colony forming unit  
 NM - necessary quantity  
 m - the highest allowed value at the case of one sample  
 M, c - "M" highest allowed value for the number "c" at the case of 5 sample`s evaluation

TT - type of test  
 A - accredited test executed at the own test laboratory  
 N - non accredited test executed at the own test laboratory  
 SA - accredited test executed under the subcontract  
 SN - unaccredited test executed under the subcontract  
 (TM) - testing outside the laboratory at the customer

\* - measurement uncertainty – sampling and analysis – determined by extension coefficient k=2 (with probability of 95%). If sample is taken by the customer uncertainty of sampling is not available.

- uncertainty given in % reflects the uncertainty from the result of measurement.

\*\* - Acceptable to consumers and no abnormal change

SL - analysis laboratory: NZ-Nové Zámky, TR-Turčianske Teplice, RK-Ružomberok, TV-Trebišov

## Disclaimer:

Laboratory is a disclaimer when the information is supplied by the customer (#) and can affect the validity of results. If the sample has been provided by the customer, the results refer to the sample as it was received. Gauges and measuring equipment used for testing were calibrated or attested in accordance with the valid metrological instructions. The above mentioned test results refer to the tested sample only! The result given in this Analytical report and marked as non accredited test shall not be a subject of accreditation. The result given in this Analytical report and marked as sub- delivery is the result of a Subcontractors gauging made under the terms and conditions of a contract concluded with him. This Analytical report shall not be reproduced except in full colour version, without written approval of the laboratory. SNAS is a Signatory to the Multilateral Agreement MRA ILAC.

Responsible for correctness:

Andrea Podušelová  
Technician worker

Worked out by: Zuzana Kubisová

Validity check of document

**Test Certificate approved by**Andrea Podušelová  
Technician worker